



**EKOTEKS**  
LABORATUVAR VE GÖZETİM HİZMETLERİ A.Ş.

**EKOTEKS LABORATUVAR ve GÖZETİM  
HİZMETLERİ A.Ş.**  
Esenyurt Firuzköy Bulvarı No:29 34325 Avcılar  
İstanbul/ TÜRKİYE



**TEST REPORT  
DENEY RAPORU**

AB-0583-T
20042076
11-20

MAE GİYİM SAN VE TİC LTD ŞTİ

*Customer name:*

KAYABAŞI MAH KAYAŞEHİR BULVARı PARK MAVERA 2 SİTESİ B2  
BLOK D 30 34494 BAŞAKŞEHİR/İSTANBUL

*Buyer name:*

-

*Contact Person:*

-

*Order No:*

-

*Article No:*

SG1389

*Name and identity of test item:*

White surgical gown.(Claimed to be; D-Lab Bioclean Isolation Gown AAMI  
Level 3 Lot Number: 2020000003.)

*The date of receipt of test item:*

10.11.2020

*Re-submitted/re-confirmation  
date:*

-

*Date of test:*

10.11.2020-16.11.2020

*Remarks:*

-

*Sampling:*

The results given in this report belong to the received sample by vendor.

*End-Use:*

-

*Care Label:*

Not specified.

*Number of pages of the report:* 3

*The Turkish Accreditation Agency (TÜRKAK) is signatory to the multilateral agreements of the European co-operation for the Accreditation (EA) and of the International Laboratory Accreditation (ILAC) for the Mutual recognition of test reports.*

*EKOTEKS LABORATUVAR ve GÖZETİM HİZMETLERİ A.Ş. accredited by TÜRKAK under registration number [AB-0583-T] for ISO 17025:2017 as test laboratory.*

*The test and/or measurement results, the uncertainties (if applicable) with confidence probability and test methods are given on the following pages which are part of this report.*



*Date*  
16.11.2020

*Customer Representative*  
Zahide TAPAN

*Head of Testing Laboratory*  
Sevim A. RAZAK  
16.11.2020


This report shall not be reproduced other than in full except with the permission of the laboratory.  
Testing reports without signature and seal are not valid.

**EKOTEKS LABORATUVAR ve GÖZETİM  
HİZMETLERİ A.Ş.**

AB-0583-T
20042076
11-20

REQUIRED TESTS	RESULT	COMMENTS
<b>PHYSICAL PROPERTIES TESTS</b>		
Water Permeability	P	
Water Resistance	P	
<p>P: Pass F: Fail R: Refer to retailer technologist. Test results were evaluated according to the ANSI/AAM1 PB70 requirements</p>		

**REMARK:** Original samples are kept for 3 months and all technical records are kept for 5 years unless otherwise specified. If requested, measurement uncertainty will be reported. But unless otherwise specified, measurement uncertainty is not considered while stating compliance with specification or limit values. The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor  $k=2$ , providing a level of confidence of approximately 95 %. The declaration of conformity was given in accordance with the Simple Acceptance Decision Rule. Tests marked (\*) in this report are not included in the accreditation schedule.

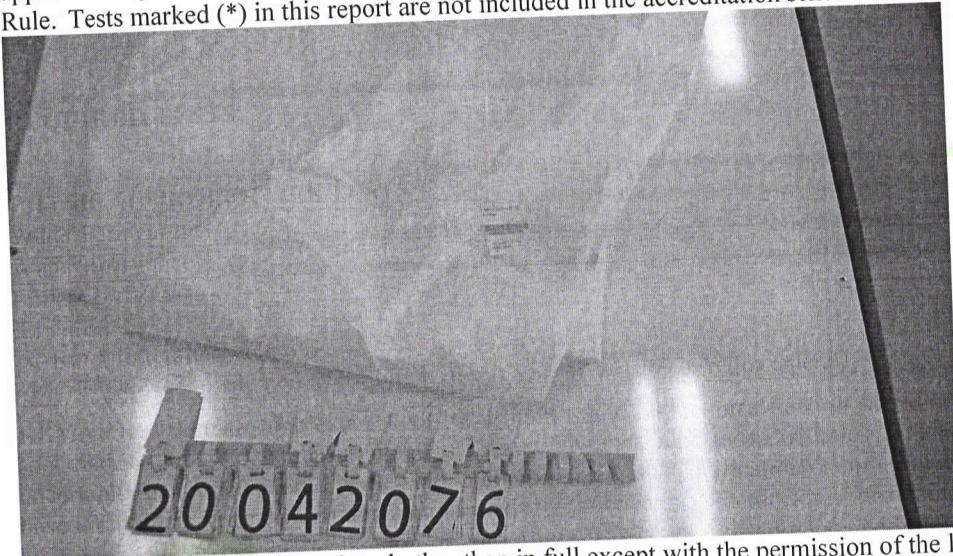

This report shall not be reproduced other than in full except with the permission of the laboratory.  
Testing reports without signature and seal are not valid.

**EKOTEKS LABORATUVAR ve GÖZETİM  
HİZMETLERİ A.Ş.**

AB-0583-T
20042076
11-20

## TEST RESULTS

### WATER RESISTANCE-IMPACT PENETRATION TEST; AATCC 42:2017

Test samples were conditioned for at least 4 hours prior to testing ( $65 \pm 5\%$  RH,  $21 \pm 2^\circ\text{C}$ ).

Water temperature :  $27 \pm 1^\circ\text{C}$

Amount of sprayed water: 500 ml

	<u>RESULT</u>	<u>REQUIREMENT</u>
Sample 1	0.02g	
Sample 2	0.01 g	$\leq 1,0$ g (Level 3)
Sample 3	0.00 g	
Average	0.01 g	

### WATER PERMEABILITY; AATCC 127:2017-OPTION 2

Hydrostatic Head Tester, Textest marka Fx 3000 model

Temperature of water  $20^\circ\text{C}$ . Pressure increase ratio 10 mbar/dk.

Performed in the conditioned room ( $21 \pm 2^\circ\text{C}$ - $65\% \pm 5$ )

	<u>RESULT</u>	<u>REQUIREMENT</u>
Sample 1	258.6 cm SS	$\geq 50$ cmSS (Level 3)
Sample 2	263.1 cm SS	
Sample 3	251.9 cm SS	
Average	257.7 cm SS	